





Test Report SL52045300091301TX

Date:October 13,2020

Page 1 of 6

GUANGZHOU BOFEITE SAFETY PROTECTIVE SUPPLIES CO.,LTD

FIRST FLOOR (PART), THIRD FLOOR(PART), FOURTH FLOOR AND FIFTH FLOOR(PART), NO.8 PLANT, XINGFU ROAD, SHAPU YINSHA INDUSTRIAL DISTRICT, XINTANG TOWN, ZENGCHENG DISTRICT, GUANGZHOU CITY

THIS REPORT CANCELS AND SUPERSEDES THE TEST REPORT NO.SL52035285718001TX DATE: 2020-09-02 ISSUED BY SGS (Shanghai) UPDATED SAMPLE INFORMATION.

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)Disposable particle filtering half mask

Sample Color : (A)WHITE

Composition : (A)Polypropylene non-woven fabric Polypropylene melt-blown fabric

Polypropylene non-woven fabric

Style No. : HT9580

Manufacturer : GUANGZHOU BOFEITE SAFETY PROTECTIVE SUPPLIES CO.,LTD

Country of Destination : Germany, Spain, France, Italy Previous No. : SL52045300091601TX

Test Performed : Selected test(s) as requested by applicant

Sample Receiving Date : Aug 13, 2020

Testing Period : Aug 13, 2020 - Sep 02, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the

sample(s) tested, for further details, please refer to the following page(s).

Based on the results of the tests reported and the previous report SL52045300091601TX issued on Oct 13, 2020, our Lab concluded that the recommendation level can be as below.

Sample No.	Recommendation Level
(A)	FFP2 NR

Signed for and on behalf of

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available or request or accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com/en/Terms-and-Conditions/Terms-a-Document.aspx. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerise to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report reter only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or, email: CN.Doccheck@sgs.com

3^{**}Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666 t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763



SL52045300091301TX

Date:October 13,2020

Page 2 of 6

Test Result

Personal Protective Equipment - Respiratory Protective Devices- Filtering Half Masks to Protect against Particles- Requirements, Testing, Marking

EN 149:2001+A1:2009

Clause 7.4 Packaging

(EN 149:2001+A1:2009 Clause 8.2)

Test Requirement	Results	Comment
Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use.	Comply	Pass

Clause 7.7 Practical Performance

(EN 149:2001+A1:2009, Clause 8.4)

Test Requirement	Results	Comment
The particle filtering half mask shall undergo practical performance tests under realistic conditions. These general tests serve the purpose of checking the equipment for imperfections that cannot be determined by the tests described elsewhere in this standard.	No imperfections	Pass

Clause 7.8 Finish of Parts

(EN 149:2001+A1:2009, Clause 8.2)

Test Requirement	Results	Comment
Parts of the device likely to come into contact with the wearer shall have no	No sharp	Pass
sharp edges or burrs.	edges or burrs	1 055



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666

t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763



SL52045300091301TX **Test Report** Clause 7.9.1 Total Inward Leakage

(EN 149:2001+A1:2009, Clause 8.5)

Date:October 13,2020

Page 3 of 6

Test Requirement	Results	Comment
The total inward leakage consists of three components: face seal leakage, exhalation value leakage(if exhalation value fitted) and filter penetration. For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25% for FFP1, 11% for FFP2, 5% for FFP3 and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than: 22% for FFP1, 8% for FFP2, 2% for FFP3	Detail refer to Appendix 1	Meet FFP1, Meet FFP2

Appendix 1: Summarization of Test Data

Inward Leakage Test Data

	Janago 100			ı	ı			
Subject	Sample	Condition	Walk(%)	Head	Head	Talk(%)	Walk(%)	Mean(%)
	No.			Side/side(%)	up/down(%)			
Zhou	1	A.R.	5.82	6.49	6.60	6.02	5.13	6.01
Luo	2	A.R.	7.48	7.68	6.32	6.52	7.41	7.08
Lu	3	A.R.	5.26	7.15	5.95	6.81	5.45	6.12
Wang	4	A.R.	5.52	5.06	4.81	5.72	4.80	5.18
Bao	5	A.R.	5.74	7.60	8.13	6.95	7.08	7.10
Ding	6	T.C.	4.88	5.47	6.32	5.67	5.08	5.48
Li	7	T.C.	6.86	7.25	7.36	7.93	6.84	7.25
Chen	8	T.C.	4.81	6.39	6.88	5.10	4.10	5.46
Song	9	T.C.	6.95	5.82	7.11	5.87	6.87	6.52
Ye	10	T.C.	7.53	7.95	5.46	8.38	7.09	7.28

Facial Dimension(mm)

<u>Subject</u>	Face length	Face Width	Face Depth	Mouth Width
Chen	125	150	120	58
Lu	115	132	107	48
Zhou	115	135	106	52
Li	125	130	107	46
Luo	125	136	100	43
Zheng	128	140	112	55
Wang	120	147	103	48
Song	120	140	100	50
Bao	130	134	104	50
Ding	134	150	110	52
Liu	120	135	117	50
Ye	126	137	105	52



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 t (86-21) 61402666

f (86-21) 64958763



SL52045300091301TX

Date:October 13,2020

Page 4 of 6

Clause 7.13 Head Harness

(EN 149:2001+A1:2009, Clause 8.4 & 8.5)

Test Requirement	Results	Comment
The head harness shall be designed so that the particle filtering half mask can be donned and removed easily.	Comply	
The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device.	Comply	Pass

Clause 7.14 Field of Vision

(EN 149:2001+A1:2009, Clause 8.4)

Test Requirement	Results	Comment
The field of vision is acceptable if determined so in practical performance	Comply	Pass
tests.		

Clause 7.18 Demountable Parts

(EN 149:2001+A1:2009, Clause 8.2)

Test Requirement	Results	Comment
All demountable parts (if fitted) shall be readily connected and secured,	Comply	Pass
where possible by hand		Fass

Test	Uncertainty
Total inward leakage	3.4%
Penetration of filter material	4.8%
Carbon dioxide content of the inhalation air	3.9%
Breathing resistance (30L/min)	5.9%
Breathing resistance (95L/min)	4.9%
Breathing resistance (160L/min)	4.3%



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3stBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐江区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 t (86-21) 61402666 f (86-21) 64958763




SL52045300091301TX

Date:October 13,2020

Page 5 of 6



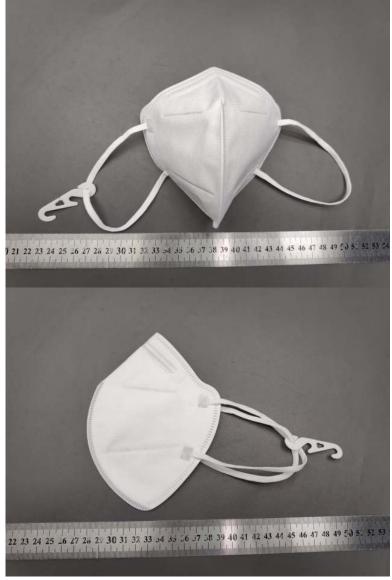



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666


t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763



SL52045300091301TX

Date:October 13,2020



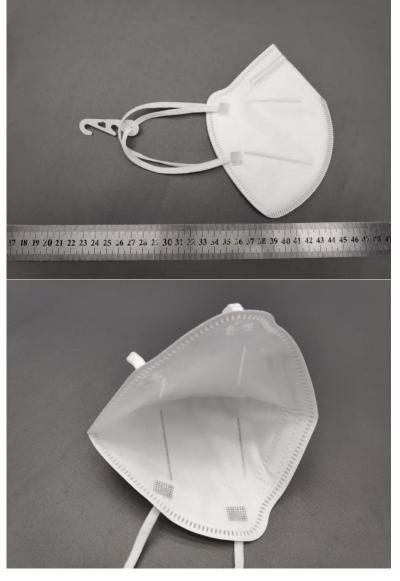

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666

t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763